

UNI 9507 probes



IDENTIFICATION

- ▶ Probes for medical gas, vacuum and instrument air distribution terminal units, type UNI 9507
- ▶ Can be supplied with straight hose connector, 90° hose connector, G 1/4" F fitting
- ▶ Instrument Air probe equipped with integrated check valve
- ▶ G 1/4" M fitting for probe dedicated to direct connection with accessories (suction equipment, flow meters)
- ▶ Made of nickel-plated brass
- ▶ Laser-engraved production lot and product code

CE MARKING

Notified body: CE 0426

CE marking in risk class II B in accordance with Legislative Decree 24 February 1997, no. 46 "Implementation of Directive 93/42/EEC, concerning Medical Devices" and further modifications

REFERENCE STANDARD

ISO 9170-1: "Terminal units for medical gas pipeline system - Part 1: Terminal units for use with compressed medical gases and vacuum"

ISO 7396-1: "Medical gas pipeline systems - Part 1: Pipeline systems for compressed, medical gases and vacuum"

UNI 9507: "Medical gas pipeline systems - Terminal units"

ISO 15001: "Anaesthetic and respiratory equipment. Compatibility with oxygen"

* Validity of the standards is referred to the current year







UNI 9507 probes

DIMENSIONS


G 1/4" FEMALE

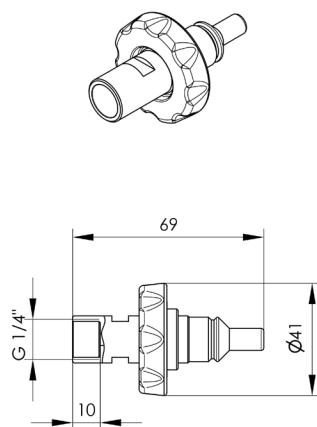


G 1/4" MALE

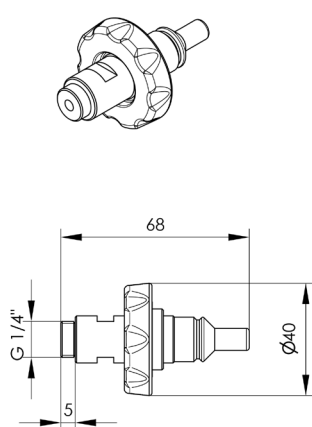

90° HOSE CONNECTOR

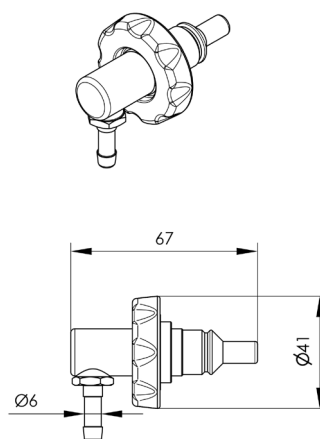



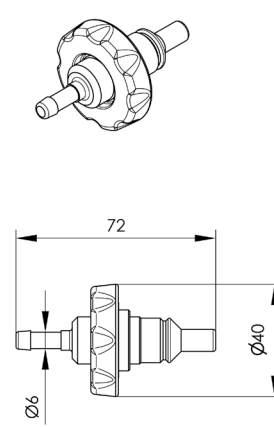




STRAIGHT HOSE CONNECTOR



- ▶ Gases: Vacuum, Oxygen, Medical Air, Nitrous Oxide, Carbon Dioxide, Instrument Air
- ▶ Storage temperature: -20 °C ÷ +60 °C

- ▶ Working temperature: +10 °C ÷ +40 °C
- ▶ Hose connector for flexible hose
Øi = 6 ÷ 6.5 mm

CODE				GAS	NOMINAL PRESSURE bar	PACKAGING		
						 type	 kg	 pcs
PF-06UF-00O2	PF-06UF-20O2	PF-06UP-00O2	PF-06UP-10O2	O ₂	4 ^{+1.0} _{-0.8}	bag	0.14	1
PF-06UF-00OV	PF-06UF-20OV	PF-06UP-00OV	PF-06UP-10OV	Vacuum	≤ -0,4	bag	0.14	1
PF-06UF-00AC	PF-06UF-20AC	PF-06UP-00AC	PF-06UP-10AC	Medical Air	4 ^{+1.0} _{-0.8}	bag	0.14	1
PF-06UF-0N2O	PF-06UF-2N2O	PF-06UP-0N2O	PF-06UP-1N2O	N ₂ O	4 ^{+1.0} _{-0.8}	bag	0.14	1
PF-06UF-0CO2	PF-06UF-2CO2	PF-06UP-0CO2	PF-06UP-1CO2	CO ₂	4 ^{+1.0} _{-0.8}	bag	0.14	1
PF-06UF-0AC8	PF-06UF-2AC8	PF-06UP-0AC8	PF-06UP-1AC8	Instrument Air	8 ^{+2.0} _{-1.0}	bag	0.14	1

