



# Terminal units type DIN 13260-2

### IDENTIFICATION

- ▶ Terminal units for compressed medical gases and vacuum, type DIN 13260-2
- ▶ Base block supplied with 20 cm length of 10 mm diameter pipe
- ▶ Base block in brass with sealing element to stop the flow
- ▶ Gas-specific nickel-plated brass socket with plastic ring
- ▶ Base block – socket connection by means of M5 screws (no. 3)
- ▶ Facility for wall mounting in recessed box, surface mount box or bed head panels and pendants
- ▶ Laser-engraved production lot and product code



### CE MARKING

Notified body: CE 0426

CE marking in risk class II B in accordance with Legislative Decree 24 February 1997, no. 46 "Implementation of Directive 93/42/EEC, concerning Medical Devices" and further modifications

### REFERENCE STANDARD


**ISO 9170-1:** "Terminal units for medical gas pipeline systems - Part 1: Terminal units for use with compressed medical gases and vacuum"

**ISO 7396-1:** "Medical gas pipeline systems - Part 1: Pipeline systems for compressed medical gases and vacuum"

**DIN 13260-2:** "Supply systems for medical gases - Part 2: Dimensions and allocation of probes and gas-specific connection points for terminal units for compressed medical gases and vacuum"

**ISO 15001:** "Anaesthetic and respiratory equipment. Compatibility with oxygen"

\* Validity of the standards is referred to the current year

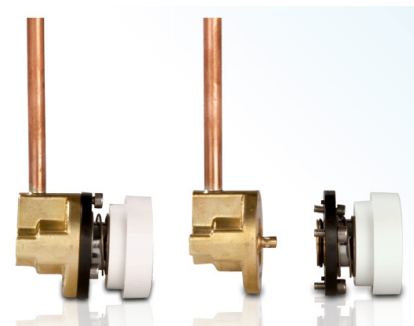

- ▶ Gases: Oxygen, Medical Air, Nitrous Oxide, Vacuum, Carbon Dioxide
- ▶ Storage temperature: -20 °C ÷ +60 °C
- ▶ Working temperature: +10 °C ÷ +40 °C


- ▶ Nominal Working Pressure:  $400^{+100}_0$  kPa ( compressed gases )
- ▶ Nominal Working Pressure:  $\leq 60$  kPa (absolute Vacuum Pressure )






## Terminal units type DIN 13260-2

## DIMENSIONS

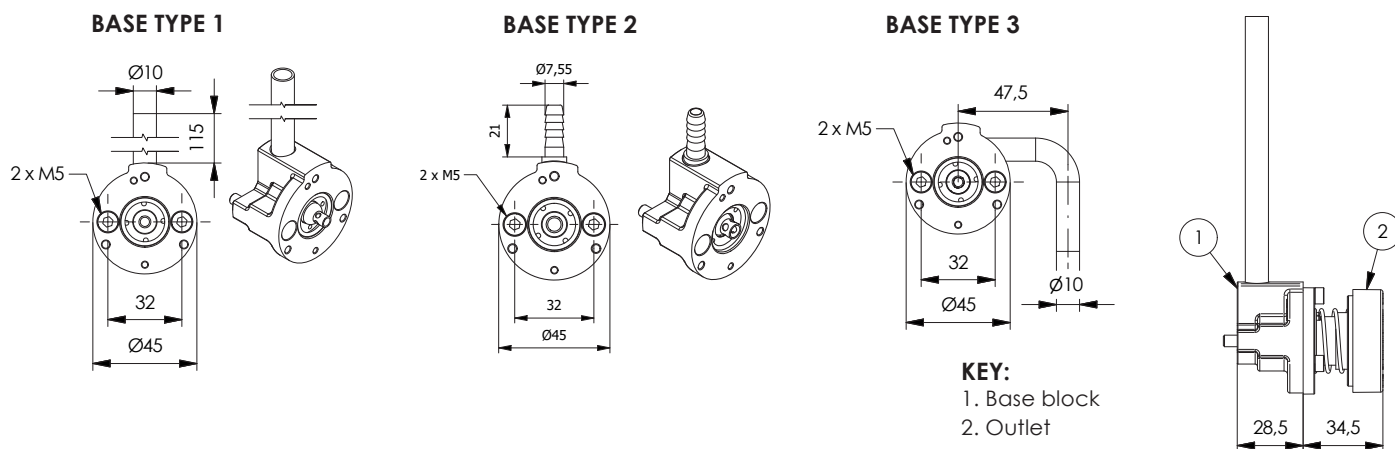

## INSTALLATION IN BED HEAD PANELS AND PENDANTS

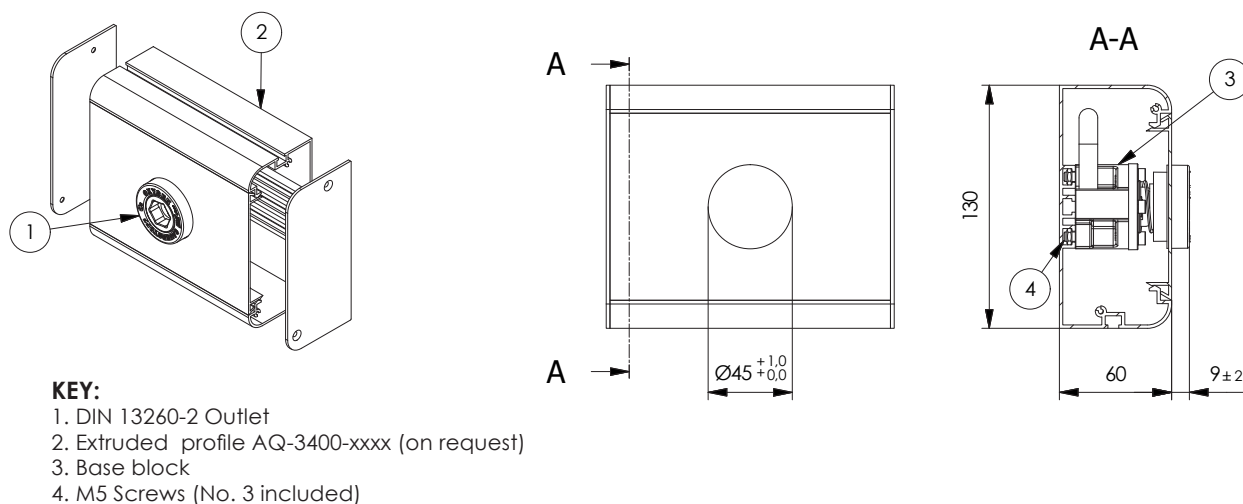

## BASE BLOCK

CODE			GAS	NOMINAL PRESSURE bar	PACKAGING		
TYPE 1	TYPE 2	TYPE 3			type	kg	pcs
PF-01DS-00O2	PF-01DP-00O2	PF-01DS-30O2	O <sub>2</sub>	4 <sup>+1.0</sup> / <sub>-0.0</sub>	bag	0.23	1
PF-01DS-000V	PF-01DP-000V	PF-01DS-300V	Vacuum	≤ -0,4	bag	0.23	1
PF-01DS-00AC	PF-01DP-00AC	PF-01DS-30AC	Medical Air	4 <sup>+1.0</sup> / <sub>-0.0</sub>	bag	0.23	1
PF-01DS-0N2O	PF-01DP-0N2O	PF-01DS-3N2O	N <sub>2</sub> O	4 <sup>+1.0</sup> / <sub>-0.0</sub>	bag	0.23	1
PF-01DS-0CO2	PF-01DP-0CO2	PF-01DS-3CO2	CO <sub>2</sub>	4 <sup>+1.0</sup> / <sub>-0.0</sub>	bag	0.23	1

## OUTLET

CODE	GAS	NOMINAL PRESSURE bar	PACKAGING		
			type	kg	pcs
PF-02DD-00O2	Oxygen	4 <sup>+1.0</sup> / <sub>-0.0</sub>	bag	0.09	1
PF-02DD-000V	Vacuum	≤ -0,4	bag	0.09	1
PF-02DD-00AC	Medical Air	4 <sup>+1.0</sup> / <sub>-0.0</sub>	bag	0.09	1
PF-02DD-0N2O	Nitrous Oxide	4 <sup>+1.0</sup> / <sub>-0.0</sub>	bag	0.09	1
PF-02DD-0CO2	Carbon Dioxide	4 <sup>+1.0</sup> / <sub>-0.0</sub>	bag	0.09	1

